



**REQUEST FOR PROPOSALS**  
**RFP No. 266 (Eng. ver.)**

**Date:** July 12, 2019

<b>Subject:</b> Request for Proposals for procurement of medical equipment for Smolinska and Kompaniivska CC (Kirovogradaska oblast) in the framework of USAID funded DOBRE.
---

From	To
<b>Global Communities, implementing agency of DOBRE Decentralization Offering Better Results and Efficiency Program financed by the United States Agency for International Development (USAID) (referred to as “BUYER” hereinafter)</b>	<b>Potential suppliers (referred to as “BIDDER” hereinafter)</b>

Proposals Submission Time and Date:	The Proposal must be submitted for the attention of:	Conditions of Payment:
By 12:00 Kyiv time on July 19, 2019, at the latest	Global Communities  International Technical Assistance Program “Decentralization Offering Better Results and Efficiency” USAID DOBRE  Address: 5b, Dilova str., Office 510, 5th Floor, Kyiv, Ukraine  Email: <a href="mailto:dobreprocurement@globalcommunities.org">dobreprocurement@globalcommunities.org</a>	<u><b>Post payment during 30 calendar days after delivery. If it is unacceptable, please indicate yours.</b></u>



## I. TERMS OF REFERENCE

A. Global Communities invites you to submit proposals for procurement of medical equipment for Smolinska and Kompaniivska CC (Kirovogradska oblast) as per the Specifications attached as Annex B1 and B2 (by separate lots). The bidders can submit their offers on all the lots, as well as on each lot separately.

## II. INSTRUCTIONS FOR POTENTIAL SUPPLIERS

### A. Form of Proposal

The proposal as well as all correspondence and documents exchanged between the Bidder and the Buyer under this RFP 266 shall be in English or Ukrainian.

The proposal must specify the following details and confirmations:

1. The Proposal should be submitted on or before the deadline for this purpose, on a company letterhead, signed by an authorized representative and include the contact details of the Bidder.
2. Conformity to technical specifications. **The Bidder must confirm that all items are responsive to, or exceed, the estimated requirements.**
3. The Proposal must be valid for at least 60 calendar days from the proposal submission deadline date.
4. Prices must be quoted in Ukrainian hryvnias (UAH).
5. Prices must be quoted without the VAT. The Buyer is exempt from taxes within the customs territory of Ukraine and shall provide a certified copy of its registration card issued by the Ministry of Economic Development and Trade of Ukraine; The Buyer shall also provide a copy of its approved procurement plan.
6. **Price for each item. The price must be quoted as a total amount on an all-inclusive basis, including delivery to Smolinska and Kompaniivska CC (Kirovogradska oblast).**
7. Eligibility for participation in the tender.
  - a. To be eligible to submit a proposal in response to this RFP, the Bidder must conform to the requirements in this RFP.
  - b. The Bidder complies with the U.S. sanctions and embargo laws, including U.S. Executive Order 13224 on Terrorist Financing and U.S. laws that prohibit transactions with, and the provision of resources and support to, individuals or entities associated with terrorism. Any person or organization taking part in this tender as a bidder or a sub-contractor must certify and confirm together with submitting other documents that the person or organization is not listed on the U.S. Department of Treasury Office of Foreign Assets Control (OFAC) Specially Designated Nationals (SDN), and is eligible for participation in the tender. Global Communities must disqualify any offers from persons or organizations listed on the said OFAC SDN list or found not to be eligible for the participation in the tender on other grounds. Companies and persons listed on the Excluded Parties List System ([www.epls.gov](http://www.epls.gov)) are not eligible for receiving funds.
8. The Buyer reserves the right to accept or reject any proposal, and to cancel the tender, reject all proposals at any time prior to the award without assuming any liability and without the duty to inform Bidders about reasons for Global Communities' actions.
9. This RFP may be modified by means of amendments. Copies of amendments shall be issued to all Bidders.



10. Any order of services to be made on the basis of this Request for Proposal shall be subject to Global Communities General Terms and Conditions of Goods and Service Procurement Contracts.

**11. The Buyer will not send any notices to Bidders with confirmation about proposals received. The Buyer will not send any notices to unsuccessful Bidders.**

**B. Evaluation Criteria**

Proposals will be evaluated in accordance with criteria listed below. First, the Buyer will evaluate proposals for meeting obligatory criteria to determine conformity to the requirements. While evaluating the proposal, the Buyer may seek additional information from any source it considers appropriate to obtain or confirm information about the Bidder’s proposal.

Following is an illustrative example of the criteria that might apply to evaluate proposals/bids.

1. Conformity to the order list specification	Acceptable/Unacceptable
2. Validity of the proposal for 60 calendar days	Acceptable/Unacceptable
3. VAT exemption	Acceptable/Unacceptable
4. Eligibility for taking part in this RFP	Acceptable/Unacceptable
5. Warranty (not less than 12 months)	Acceptable/Unacceptable
<b>6. Price</b>	<b>40 points</b>
<b>7. Quality of proposal</b>	<b>15 points</b>
<b>8. Terms of delivery</b>	<b>15 points</b>
<b>9. Payment terms - Post payment during 30 calendar days after delivery</b>	<b>30 points</b>

**C. Questions with regard to this RFP**

All clarification requests shall be sent in writing to the addresses specified hereinabove by **12:00 pm on July 17, 2019**, at the latest. Please refrain from personal visits and phone calls. Any information provided to one Bidder with regard to this RFP will be made available to all Bidders.

Sincerely,

Global Communities  
“Decentralization Offering Better Results and Efficiency” International Technical Assistance Program  
USAID DOBRE



**Annex A: Proposal Requirements**

**1. Please confirm next mandatory requirements:**

Conformity to the order list specification	Acceptable/Unacceptable
Validity of the proposal for 60 calendar days	Acceptable/Unacceptable
VAT exemption	Acceptable/Unacceptable
Eligibility for taking part in this RFP	Acceptable/Unacceptable
Warranty (12 months)	Acceptable/Unacceptable
Post payment during 30 calendar days after delivery.	Acceptable/Unacceptable




**If payment conditions are unacceptable, please indicate yours**






**2. General information**



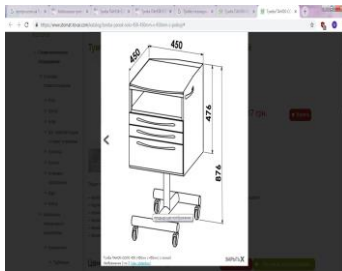

**Please fill the table with general information**




Company name:			
Code for Uniform State Register of Enterprises and Organisations (for legal entities) or Registration number of taxpayer's account (for private entrepreneur)			
Address:	Postal code:	City:	Country:
P. O. Box and mailing address			
Phone number:			
E-mail:			

**Annex B1: Specification. Medical equipment for Kompaniivska CC.**







##	Items description	Images*	Unit of measure	Q-ty
1	<p>Dental unit "Siger U200" or equivalent. Basic equipment includes: dental fitting mounted on the chair. Touchpad (one touch) control panels at the doctor's and assistant's table.</p> <p><u>Doctor's block:</u> a three-functional doctor's gun; Midwest turbine hose or equivalent, without backlighting. The place for a tool with a lower socket or an upper lever.</p> <p><u>Assistant block:</u> three-function assistant gun. Ejector or Wet line. Ejector vacuum cleaner or Wet line.</p> <p>Patient armchair: anatomical form with seamless upholstery. Electromechanical with memory function for 5 positions. Emergency stop system of the chair. Articulating headrest for adult and children's reception. Clean water system. Armchair Siger or equivalent with left armrest. Foot control pedal with joystick. Lighting operating light emitting diode (9 000 - 33 000 Lux).</p>	 <p>www.dentpro.com.ua</p>	pcs.	1
2	<p>Bollard with a shelf "Punk - Solo 450" or equivalent. Dimensions according to the drawing. Color is white.</p>	 	pcs.	1

				
3	<p>The shade "Medilux 4HF" or the equivalent.</p> <p><u>Specifications:</u> low energy consumption, no magnetic and electric fields. Adjustable height - fastening on a chain. Protective coating of the upper part of the luminaire. The infrared filter prevents thermal radiation, frees up the eye, and gives intense shade daylight. Material: compressed aluminum profile. Color: white (powder varnish RAL7047). Lighting: 5 000 lux / 2.3 m. Color temperature: 5 500 K RA85. Overall dimensions, mm: 1570x670x90. Weight, kg: 17. Tube power: 4 x 58W. Voltage: 220V. Lamp life: 16,000 working hours.</p>		pcs.	1
4	<p>Sterilizer "GP-40" or equivalent.</p> <p><u>Specifications:</u> Dimensions: 730x500x475mm. Camera volume: 40l. Power supply: 220V, 50Hz. Power not more than 1.9 kW.</p>		pcs.	1
5	<p>Tip turbine "SOCO SCHG 18-TP4" or equivalent.</p> <p><u>Specifications:</u> 4-channel connection. (Midwest, M4). The material of the case is stainless steel. Clip type - button. Autoclave treatment - autoclaving at 135 ° C. Spray single - is. The type of beams - FG Ø1,6 mm (turbine). Bearing type - steel. Purpose - universal, orthopedic. Local illumination - no.</p>		pcs.	1
6	<p>Tip turbine "AR Led Generator" or equivalent.</p> <p><u>Specifications:</u> Clip type - push button. Four-channel connection (Midwest, M4 or equivalent), multiflex, fast-moving (bayonet). Local illumination is there. Stand alone with generator, LED. Purpose - universal, orthopedic. Type of</p>		pcs.	2

	boring FG Ø1,6mm (turbine). Bearing type - ceramic. Autoclave treatment - autoclaving at 135 ° C. Case material - stainless steel. Four-point spray (internal) - there is.			
7	<p>Corner tip "AP RA 1: 1" or the equivalent.</p> <p><u>Specifications:</u> Reduction 1: 1, direct transmission. Clip type - button. Local illumination - no. Appointments - therapeutic, universal. Borland type - CA / RA Ø2,35mm (angular). Connection - for a micromotor. Bearing type - steel. Autoclave treatment - no. The material of the case is stainless steel. Spray (external, internal) - no.</p>		pcs.	1
8	<p>Tip "NZTM-40" or the equivalent.</p> <p><u>Specifications:</u> transmission ratio - direct transmission 1: 1. For HP bore (Ø2.35 mm). Max speed: 40,000 rpm Local illumination - no, spray - no, autoclave treatment - no. Body material - steel.</p>	 <p>www.dentpro.com.ua</p>	pcs.	1
9	<p>Photo lamp "Calcizer Translux" or equivalent.</p> <p><u>Specifications:</u> The advanced 360 ° swivel beam angle provides better access to the molar areas. One-button operation. LED indicators point to a program change. The material of the case is plastic. Luminous flux power, mW / cm<sup>2</sup>: 1000-1500. Light source LED (LEDs). Photopolymerizer properties - battery (wireless).</p>	 <p>www.dentpro.com.ua</p>	pcs.	1
10	<p>Oil-free compressor "Granum-180" or equivalent.</p> <p><u>Specifications:</u> performance - 200 l / min; receiver volume - 45 l; noise level - 60-70 dBa; power - 2x0,8 kW; working pressure - 6-8 bar; dimensions - 48x110x87 cm, weight - 75kg.</p>		pcs.	1

<p><b>11</b></p>	<p>Ultrasonic sink "SD-4800" or equivalent - produces ultrasonic cleaning of hand tools before the sterilization procedure, in particular tools with openings, recesses or rotary joints (scissors, cuticles, tongs, pliers, etc.), saws, nozzles for mills, boron, cutters, needles for tattooing, but only metal products.</p> <p><u>Specifications:</u> gross weight: 2.15 kg. Net Weight: 1.75 kg. Interior dimensions 170 × 135 × 65 mm. Exterior dimensions: 230 × 180 × 160 mm. Power: 100 W (220 V). Power supply: AC 220-240V, 50 / 60Hz. Timer: 5 cycles with a digital display. Volume: 1.4L. Material: stainless steel SUS304. Ultrasonic frequency: 42 kHz.</p>		<p>pcs.</p>	<p>1</p>
<p><b>12</b></p>	<p>Straight elevator - intended for extraction of the roots of single-root teeth or disconnected roots of multi-root teeth of the upper jaw, as well as extraction of teeth that lie outside the dental arc and rarely - mandibular large root teeth.</p> <p><u>Specifications:</u></p> <ul style="list-style-type: none"> <li>- the width of the working surface - 4.2 mm;</li> <li>- pear-shaped pen;</li> <li>- handle with a plurality under the finger;</li> <li>- surgical stainless steel;</li> <li>- an autoclave tool.</li> </ul>		<p>pcs.</p>	<p>10</p>
<p><b>13</b></p>	<p>Elevators (left) - designed to remove the roots of the teeth of the lower jaw and large root tooth. Surgical Elevator 720/10 or equivalent:</p> <ul style="list-style-type: none"> <li>- corner; left;</li> <li>- the width of the working surface - 3.0 mm;</li> <li>- pear-shaped pen;</li> <li>- handle with a plurality under the finger;</li> <li>- surgical stainless steel;</li> <li>- an autoclave tool.</li> </ul>		<p>pcs.</p>	<p>5</p>



14	<p>Elevators (right) - designed to remove root teeth of the mandible and large root tooth. Surgical Elevator 720/11 or equivalent:</p> <ul style="list-style-type: none"> <li>- corner; right;</li> <li>- the width of the working surface - 3.0 mm;</li> <li>- pear-shaped handle for more convenient and reliable seizure;</li> <li>- surgical stainless steel;</li> <li>- an autoclave tool.</li> </ul>		pcs.	5
15	<p>A set of surgical elevators (9 pcs.), Medesy 686 / SET or equivalent. The kit includes:</p> <ul style="list-style-type: none"> <li>- Surgical elevator 3.0 mm straight with a curve back;</li> <li>- Surgical elevator 3.6 mm straight with a curve back;</li> <li>- Surgical elevator 4.2 mm straight with a curve back;</li> <li>- Surgical elevator 3.0 mm straight;</li> <li>- Surgical elevator 3.0 mm, left corner;</li> <li>- surgical lift 3.0 mm, angular right;</li> <li>- Surgical elevator 2.2 mm straight;</li> <li>- Surgical elevator 2.2 mm, left corner;</li> <li>- Surgical elevator 2.2 mm, right corner;</li> <li>- surgical stainless steel;</li> <li>- an autoclave tool.</li> </ul>		pcs.	1
16	<p>Anatomical anchor removers, set (10 pcs.) Dental Product or equivalent.</p>		pcs.	2
17	<p>Scissors Surgical, Straight, Slim Line or equivalent, 115mm.</p>		pcs.	10
18	<p>Bath for disinfection of instruments "Bode", 10 liters or equivalent. Design: bath with lid and PVC insert. The color is white. Cover: transparent. Useful volume: 10 liters, with serious markings. Dimensions in mm: 390 x 290 x 170.</p>		pcs.	1
19	<p>Disinfection detergent for tools and surfaces «Bacillol AF», 5l. or equivalent. Ready solution for instant disinfection of surfaces in 30 seconds, as well as medical, dental and cosmetic instruments and medical products.</p>		pcs.	1



<b>20</b>	Surg Dentist Chair or equivalent. The chair has a metal chrome base, five wheels. The height of the seat and the tilt of the back should be adjusted. There must be a reliable pneumatic spring and seamless upholstery.	 <small>www.dentpro.com.us</small>	pcs.	1
-----------	--	---	------	---











**\* note: images are provided for information only, offers should include similar items.**

**Annex B2: Specification. Medical equipment for Smolinska CC.**


##	Items description	Images*	Unit of measure	Qty
1	<p>Audiotes-A1 diagnostic audiometer or equivalent.</p> <p><u>Specifications:</u>            Frequency range: 0,125 - 8 kHz (possibly up to 16 kHz). Range of output levels: by air conductivity; on bone conduction. Standard for class 1 audiometers: from -10 to 120 dB at medium frequencies, from -10 to 80 dB at mid-range frequencies. The type of main telephones TDH39, HDA200, HDA280 and others. Type of bone vibrator Radio Ear B-71 (planned B-81). Type of output signals - tone, tonal pulse. Narrowband third octave noise, broadband noise. Number of channels (independent) - 2. Language audiometry, language tests are recorded either in the internal memory of the device, or read from an external SD-card, a USB drive. The display type is 7", 65K colors, resolution 800x480, touch panel. Dimensions: 290x200h77mm. Ports: 4 USB ports, RG45 Ethernet, SD card. Level controllers. Print results. Direct printing to color inkjet printers (via a connected computer). Possible direct printing on PCL-compatible laser or inkjet printers. Built-in amplifiers of free sound field. High-quality amplifiers with 20 watts RMS sound power. Extramural audiometry. Maximum levels of intensity through main telephones are 110 dB, broadband noise is 105 dB, bone marrow is 75 dB. Indicators of the output level of the rms value. Test signals - tone signals, trill (sinus or triangular modulation), pulse signals. Setting options through the menu. Masking is a narrow-band third-octave noise, white noise. Outputs - 2 independent channels. Main phones, bone vibrator, free sound box, internal phones, linear output. Acoustic converters-audiometric phones TDH39, HDA280 and others. Bid phone B71 - standard equipment. Passive speakers: 8 ohms - 4 ohms.</p>		pcs.	1

<p>2</p>	<p>FITAL BIOMED BF500 monitor or equivalent. Mode of operation - pulse-wave. Operating frequency of the sensor (1 MHz ~ 3 MHz) ± 10%. P<sub>-</sub> (Negative Peak Sound Pressure) &lt;1 MPa. I<sub>ob</sub> (Intensity of output beam) &lt;20mW / c m<sup>2</sup>. I<sub>spta</sub> (Average intensity of spatial peak) &lt;100mW / c m<sup>2</sup>. Measurement range ChSSp 50ud. / Min ~ 210ud. / min Measurement accuracy ChSSp ± 1ud. / min TOCO measuring range 0 ~ 100%. Non-linear TOCO ± 8% error. Printing speed 1cm / min, 2cm / min, 3cm / min. Classification IEC60601: Class I, Type CF, Type BF. Display: color, 12.1-inch, 800x600. Thermal paper: width 150mm. Power supply: 100 - 240V ~, 50/60 Hz, 80 VA. Battery: Li, 14.8 V / 4400 mA * year. Length × Width × Height: 352 × 269.5 × 101mm. Weight: 5kg.</p>		<p>pcs.</p>	<p>1</p>
<p>3</p>	<p>Transport SHVD A II 6000 A or equivalent - a machine pcs.historical ventilation of lungs for emergency emergencies. It can be used in ambulance cars, as well as in resuscitation and intensive care units. Features of the machine: IPPV ventilation modes or spontaneous ventilation; innovative voice guidance system; compact design and weight of only 0.6 kg. The Li-ion battery provides continuous operation for 10 hours.</p>		<p>pcs.</p>	<p>1</p>
<p>4</p>	<p>A set of equipment and tools for proctology, BRIGHTFIELD (13 items) or equivalent.</p>	<p>Halogen light source</p>  <ul style="list-style-type: none"> <li>- Light source - halogen lamp</li> <li>- Power of a halogen lamp 250 W</li> <li>- Lighting 1800 000 LK.</li> <li>- Color temperature 3200 K</li> </ul> <p>Lightweight Ø 4 mm, L = 3000 mm</p> 	<p>pcs.</p>	<p>1</p>



		Rectoscope, Ø 20mm, L = 250mm 			
		Rectoscope, Ø 20MM, L= 123 MM 			
		Cover glass 			
		Aspiration tube 			
		Flexible biopsy forceps 7Fr, L = 370 mm 			
		Flexible biopsy forceps 7Fr, L = 370 mm 			
		Flexible biopsy forceps 7Fr, L = 370 mm 			
		Flexible scissors 7Fr, L = 370 mm 			
		Cotton Applicator 			
		Suction Catheter 			



		Brush for cleaning proctology			
					

**\* note: images are provided for information only, offers should include similar items.**



**Annex C1: Detailed Budget. Medical equipment for Kompaniivska CC.**

No.	Goods/Service Item	Quantity	Terms of Delivery (working days)	Warranty (months)	Price in Hryvnia (UAH, without VAT)	Total, in Hryvnia (UAH, without VAT)
1.						
2.						
3.						
4.						
5.						
6.						
Total in UAH, without VAT						

**Annex C2: Detailed Budget. Medical equipment for Smolinska CC.**

No.	Goods/Service Item	Quantity	Terms of Delivery (working days)	Warranty (months)	Price in Hryvnia (UAH, without VAT)	Total, in Hryvnia (UAH, without VAT)
1.						
2.						
3.						
4.						
5.						
6.						
Total in UAH, without VAT						

Signature:

(Seal)

Date: